


IAEA standards

Calibration deviation to reference values

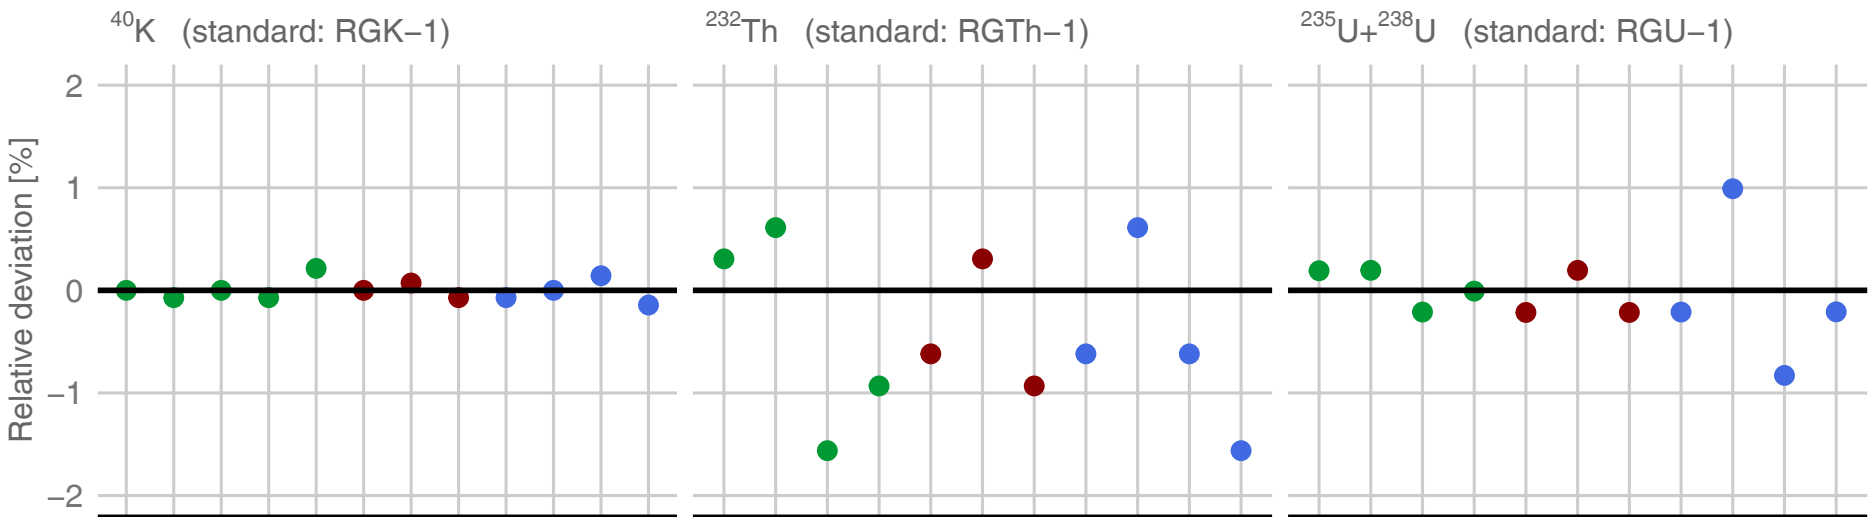

Measured for ~24 h on μDose -device ● 005 – Ahnert ● 006 – Bremer ● 007 – Rohdenburg

Relative deviation = (Experimental value – IAEA reference value) / IAEA reference value.