Technical note: Darkroom lighting for luminescence dating laboratory

Marine Frouin[1], Taylor Grandfield[1], William Huebsch[1], Owen Evans[1]

[1]Department of Geosciences, University of Stony Brook, USA

Correspondence to: Marine Frouin (marine.frouin@stonybrook.edu)

Abstract. An optimal lighting setting for the darkroom laboratory is fundamental for the accuracy of luminescence dating results. Here, we present the lighting setting implemented in the new Luminescence Dating Research Laboratory at Stony Brook University, USA. In this study, we performed spectral measurements on different light sources and filters. Then, we measured the optically stimulated luminescence (OSL) signal of quartz and the infrared stimulated luminescence (IRSL) at 50°C (IR_{50}) as well as post-IR IRSL at 290°C ($pIR-IR_{290}$) signal of potassium (K)-rich feldspar samples exposed to various light sources and durations.

Our ambient lighting is provided by ceiling fixtures, each equipped with a single orange light-emitted diode (LED). In addition, our task-oriented lighting, mounted below each wall-mounted cabinet and inside the fume hoods, is equipped with a dimmable orange LED stripline.

The ambient lighting, delivering 0.4 lux at the sample position, induced a loss of less than 5% (on average) in the quartz OSL dose after 24 h of exposure, and up to 5 % (on average) in the IR_{50} dose for the K-rich feldspar samples, with no measurable effect on their $pIR-IR_{290}$ dose. The fume hood lighting, delivering 1.1 lux at the sample position, induced a dose loss of less than 5 % in quartz OSL and K-rich feldspar IR_{50} doses after 24 h of exposure, with no measurable effect on their $pIR-IR_{290}$ dose. As light exposure during sample preparation is usually less than 24 h, we conclude that our lighting setting is suitable for luminescence dating darkrooms, it is simple, inexpensive to build, and durable.

1 Introduction

Luminescence dating techniques enable evaluation of the time that has elapsed since crystallized mineral grains, such as quartz and feldspar, were last exposed to sunlight or high temperature. Hence, a fundamental requirement of the method is that the light-sensitive traps in mineral grains must have been entirely emptied in the past and remained unexposed to light until laboratory measurement (Aitken, 1998). During sample collection in the field and sample preparation in the laboratory, precautions should be taken to preserve the integrity of the samples using controlled lighting conditions; otherwise, there is a severe risk of reducing the dating signal (i.e., luminescence signal) and hence the apparent age (i.e., deposition time) of the mineral grains. For quartz grains, the shorter wavelengths (less than 360 nm) are most effective in evicting electrons from traps. For K-rich feldspar grains, the bleaching resonance is centered at 860 nm. For quartz and feldspar grains, dim lighting conditions in the orange-yellow to red wavelength provide minimal signal loss over a limited time (Aitken, 1998). Within this

large wavelength range, each luminescence dating laboratory worldwide defines its lighting conditions. In fact, only a few laboratories have reported measurements of their lighting conditions (e.g., Spooner, 2000; Huntley and Baril, 2002, Lindvall et al., 2017; Sohbati et al., 2017, 2021) and their effect on the mineral samples.

Here we report on the lighting conditions implemented in the new Luminescence Dating Research Laboratory at Stony Brook University. First, we performed spectral measurements on different light sources and filters. Then, we measured the dose loss of quartz and potassium (K)-rich feldspar samples after exposure to various light sources and times.

2 Samples and Instrumentation

Spectral measurements were performed using a Qmini Wide VIS (AFBR-S20M2WV) spectrometer with a spectral range of 212–1035 nm (sensitivity optimized at ~500 nm) and a spectral resolution at 1.5 nm equipped with an optic fiber P400-1-UV-VIS400. The calibration of the spectrometer was performed in May 2019. All spectra were measured over a total integration time of 2 s. The amount of light on the laboratory benchtops was measured with a luxmeter Dr.meter LX1330B digital illumination/light meter.

In this study we used two quartz samples and two feldspar samples. One of the quartz sample is the calibration quartz (180-250 µm, batch #118 and #123; Hansen et al., 2015). The second quartz sample (SB27) was collected from the middle palaeolithic site of Oscurusciuto (Italy) and had a natural average dose of 133±5 Gy (n=14) (publication in prep). The feldspar samples SB36 and 44 were from the last glacial cycle and collected on Long-Island, NY. Sample SB36 had a saturated pIR-IR$_{290}$ dose (2D$_0$=328±10 Gy, n=3). Sample SB44 had an average pIR-IR$_{225}$ dose of 49±1 Gy (n=11, not fading corrected) and a pIR-IR$_{290}$ dose of 67±3 Gy (n=12).

Coarse grain (180-250 µm) fractions were dispensed on 10-mm-diameter aluminium discs (quartz) and cups (feldspar) with a silicone oil adhesive of 4-mm-diameter. Sixty aliquots per sample were prepared.

The luminescence measurements were performed on a Risø TL/OSL DA-20 reader equipped with a photomultiplier tube ET PDM9107-CP-TTL and a ^{90}Sr/^{90}Y source delivering a dose of 0.106 ± 0.003 Gy.s^{-1} to the material deposited on a disc. The luminescence signal from the quartz grains was stimulated with blue diodes emitting at 470±30 nm and detected through a combination of a 2.5- and 5-mm-thick Hoya U-340 glass filters (transmission between ~290–370 nm). The infrared stimulated signal from the K-rich feldspar grains was stimulated with LEDs emitting at 850±30 nm, and the luminescence signal was detected through the so-called blue filter pack composed of a 3-mm-thick Schott BG3 and a 2-mm-thick Schott BG39 filter (detection window centred on 410 nm).

A standard multi-grain Single-Aliquot Regenerative (SAR) procedure was used for the dose determination. After the measurement of the natural OSL signal, the aliquots were subjected to regenerative-dose cycles (including a duplicate dose and zero dose). The SAR protocol was applied to quartz samples with a preheat of 220°C for 10 s, and a cutheat of 180°C. The quartz OSL signal was measured for 40 s at 125°C prior to heating at a higher temperature for the quartz samples. The net

intensity of the blue luminescence signal was integrated over the first 0.8 s after subtracting the background signal derived from the last 8 s of stimulation. For feldspar, equivalent doses were measured using SAR protocols exploiting the IRSL signal measured at low temperature and referred to as the IR_{50} protocol (Huntley and Lamothe, 2001), as well as the post-infrared-infrared luminescence signal measured at high temperature and referred to as the pIR-IR$_{290}$ (Thiel et al., 2011). Prior to the IRSL stimulation, standard preheat conditions were applied at 250°C for 60 s and 320°C for 60 s, for the IR_{50} and pIR-IR$_{290}$ protocols, respectively. Both luminescence signals were integrated over the first five seconds of stimulation, and the background was taken from the last 10 s of stimulation. For quartz and feldspar samples, the growth curve was fitted with a single saturating exponential function. The uncertainties on an individual dose have been determined using classical rules of error combination using the Analyst software (Duller, 2007), a further systematic uncertainty of 2 % was added in quadrature to each uncertainty value to account for calibration errors and machine reproducibility.

3. Methodology

3.1 Lighting condition

The decay of luminescence in both quartz and feldspar can be induced by any wavelength of solar radiation. More precisely, the maximum bleaching rate of the quartz OSL signal is induced by short wavelength (in the UV-blue-green region), while feldspar IRSL signals have their bleaching resonance in the long wavelengths (in the red-infrared region). Therefore, finding an optimum lighting condition for both quartz and feldspar is difficult. Some luminescence laboratories use red bulbs or red fluorescent tubes, which are particularly well adapted for quartz (Sutton and Zimmerman, 1978). Lamothe (1995) reports that restriction to the wavelength region 650-600 nm can be obtained from a white fluorescent tube using three layers of Lee 106 filters (i.e., deep red) and an infrared trimming glass filter. However, Lindvall et al. (2017) reports a loss of 3 to 21% of the quartz luminescence signal intensity after 24 h of exposure to the red wavelength. For feldspar, there is an optimum at 620-540 nm in the yellow part of the spectrum (Huntley and Baril, 2002, their Fig.1). Orange-yellow wavelength can be obtained using a low-pressure sodium vapor lamp with appropriate yellow filters to block the blue to ultraviolet emissions (Spooner, 1993, 2000). Sohbati et al. (2017, 2021) also observed that using amber light-emitting diodes (LEDs) with an emission peak at 594 nm, quartz and feldspar lost only between 1 to 3 % of luminescence signal intensity after 48 h of exposure.

On another note, a comfortable laboratory illumination level is required for the safety of those spending long hours working in the darkrooms. In low light conditions (e.g., moonless night), human eyes have a maximum sensitivity at 507 nm (in the blue-green region), and red light is almost invisible. Green wavelength cannot be used in our laboratory as our lighting environment, as it bleaches the quartz OSL signal. However, the closest solution and, therefore our best compromise is the orange-yellow wavelength, similar to what was recommended by Sobhati et al. (2017, 2021).

3.2 Bleaching test procedure

All aliquots were bleached for five days in a solar simulator (UVACUBE400) equipped with a SOL500 lamp filtered with an H1 filter glass (transmission range from 315 nm to 800 nm). Quartz samples received an artificial beta dose of 5 Gy (calibration quartz) or 20 Gy (SB27). K-rich feldspar samples (SB36 and 44) received an artificial beta dose of 70 Gy. All the aliquots were placed at different locations in the darkrooms for 24, 72, 240, and 720 h, and their remaining dose was measured and normalized by the given dose. Noting that 720 h exposure is an unrealistic exposure time for sample preparation in the laboratory, nevertheless, we wanted to investigate the effect of extremely long exposure.

To monitor the bleaching effect of the ceiling fixtures, the aliquots were placed on a benchtop at a workstation. To monitor the bleaching effect of the dimmable LEDs, we fixed the light intensity at 20 % and 30 % of their maximum intensity inside our two fume hoods with a black benchtop, and at 20 % inside our fume hood with a white benchtop.

In nature, the quartz OSL signal bleaches faster than the K-feldspar signals, and the K-feldspar IR_{50} signal bleaches faster than the K-feldspar $pIR-IR_{290}$ signal. Therefore, the OSL and IR_{50} signals are key for monitoring the bleaching effect of our laboratory darkroom lights, rather than the $pIR-IR_{290}$. The IR_{50} signal is, however, and contrary to the $pIR-IR_{290}$ signal, affected by anomalous fading, which is a loss of luminescence signal through time. To account for fading and overcome any laborious fading correction, we measured all the aliquots 720 h after the initial beta irradiation. In practice, a set of aliquots was given a dose of 70 Gy, and then stored in the dark for 720 h, while another set of aliquots was exposed to a light source for 24 h and then stored in the dark for 696 h, while another set of aliquots was exposed for 72 h, and then stored in the dark for 648 h, and so on. Assuming that all the aliquots are affected by the same fading rate after one month, any tendency that we will observe as a result of our bleaching test is assumed to be the only effect of the light exposure.

4 Results

4.1 Spectral analysis

We measured the emission spectrum of three light sources: a red LED PAR38, a deep orange single LED, and a dimmable deep orange LED stripline. Details on the LEDs are reported in Table 1. The PAR38 LED emits a peak wavelength at ~600 nm (FWHM ~84 nm) with a large tail in both the short and the long wavelength emissions and a low-intensity peak at ~452 nm, in the blue region of the spectrum (Fig. 1a). The single LED emits a peak wavelength of 594 nm and the stripline of LEDs emits a peak wavelength at 596 nm (Fig. 1a). Both peaks are narrow with a FWHM of ~ 14 nm. Contrary to the red PAR 38 LED, the single and stripline LEDs results are the closest to our preferred conditions.

Table 1. LED details given by the manufacturers.

Type	Name	Lumens	Wavelength (peak)	Wavelength (dominant)	FWHM	Viewing angle	CIE xy	Company (ref)

Ambient	Cree XLamp XP-E2 LEDs	Flux: 73.9 lm (min.) @ 350mA	590 nm	590 nm	5 nm	110	-	LEDsupply (CREEXPE2-COL-X 1-Up)
Fume Hood	SimpleColor™ Amber LED Strip Lights	Per ft: 185 lm @ 365 mA @ 12V DC	592 nm	590 nm	15.5 nm	110	0.5811,0.4181	Waveform lighting (7041.592)with dimmer

120

121

(a)

(b)

(c)

(d)
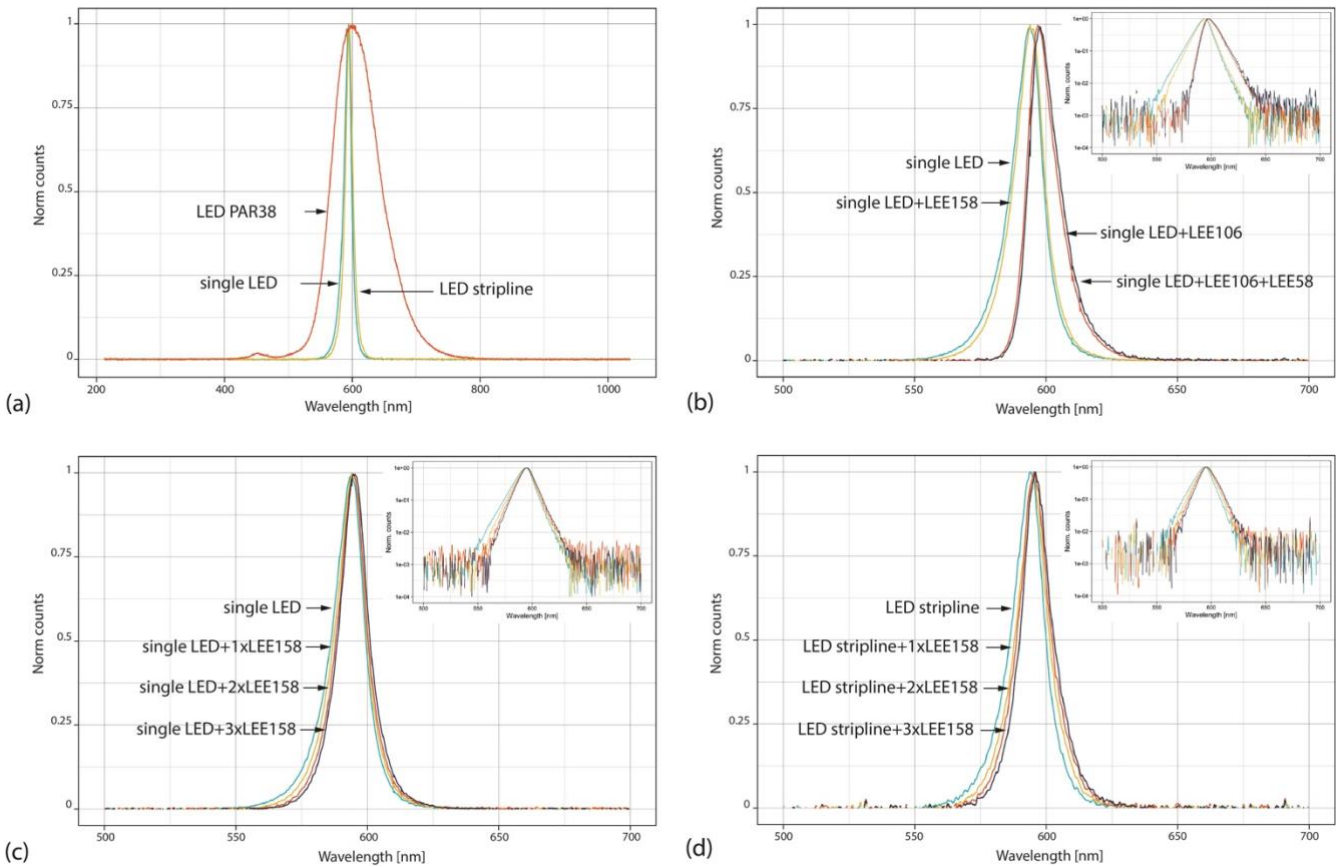
Figure 1: The normalized emission spectra of (a) the LED PAR38, single LED, and LED stripline, (a) the single LED though different long-pass filter combination, (c) the single LED through layers of the 158 Deep Orange LEE filter (LEE158), (d) the LED stripline through layers of the LEE158.

The single LED and the stripline LEDs have, however, a tail in the short wavelengths starting at ~530 nm in the green region of the spectrum. To reduce this short wavelength emission, we measured the emission spectrum of the single LED with

129 a series of long-pass filters: 106 primary red LEE, which has a cut-off at 580 nm, and 158 Deep Orange LEE, which has a cut-

130 off at 530 nm. As expected, the primary red filter successfully removed the short-wavelength emission (Fig. 1b), however, the

131 peak wavelength shifted from 594 nm to 597 nm, and a tail in the long wavelength emissions appeared (up to 640 nm). With

132 the orange filter, the tail in the short wavelengths is slightly reduced, while the rest of the LED emission spectrum remains the

133 same (Fig. 1b). Using both filters simultaneously results in an emission spectrum similar to the one obtained with the primary

134 red filter (Fig. 1b). In order to narrow the emission band of the single LED, we measured its spectrum with additional layers

135 of 158 Deep Orange LEE long-pass filter. Figure 1c shows that adding one, two, or three layers of orange filter significantly

136 contributes to reducing the short-wavelength emission while slightly increasing the long-wavelength emission. With three

137 layers of orange filter, the single LED peak wavelength is at 595 nm (FWHM ~13 nm). Similarly, adding three layers of 158

138 Deep Orange LEE long-pass filter in front of the stripline LEDs successfully removes the green emission (Fig. 1d), while the

139 peak emission remains at 596 nm (FWHM ~13 nm).

140   Our ceiling lighting consists of line track fixtures made of aluminium alloy placed at ~1.70 cm from the benchtop

141 (Fig. 2a). Each fixture has a single orange LED covered by three layers of 158 Deep Orange LEE filters and a transparent

142 acrylic glass (1-mm-thick). We checked that the transparent acrylic glass does not change the light spectrum. Inside the fume

143 hoods, we used the dimmable LED stripline covered by three layers of 158 Deep Orange LEE filters and a transparent

144 acrylic glass (3-mm-thick), placed at 1.20 cm from the benchtop (Fig. 2b-d). The same stripline of dimmable orange LEDs

145 with 158 Deep Orange LEE filters was fixed under the wall-mounted cabinets, and 0.50 cm from the benchtop.
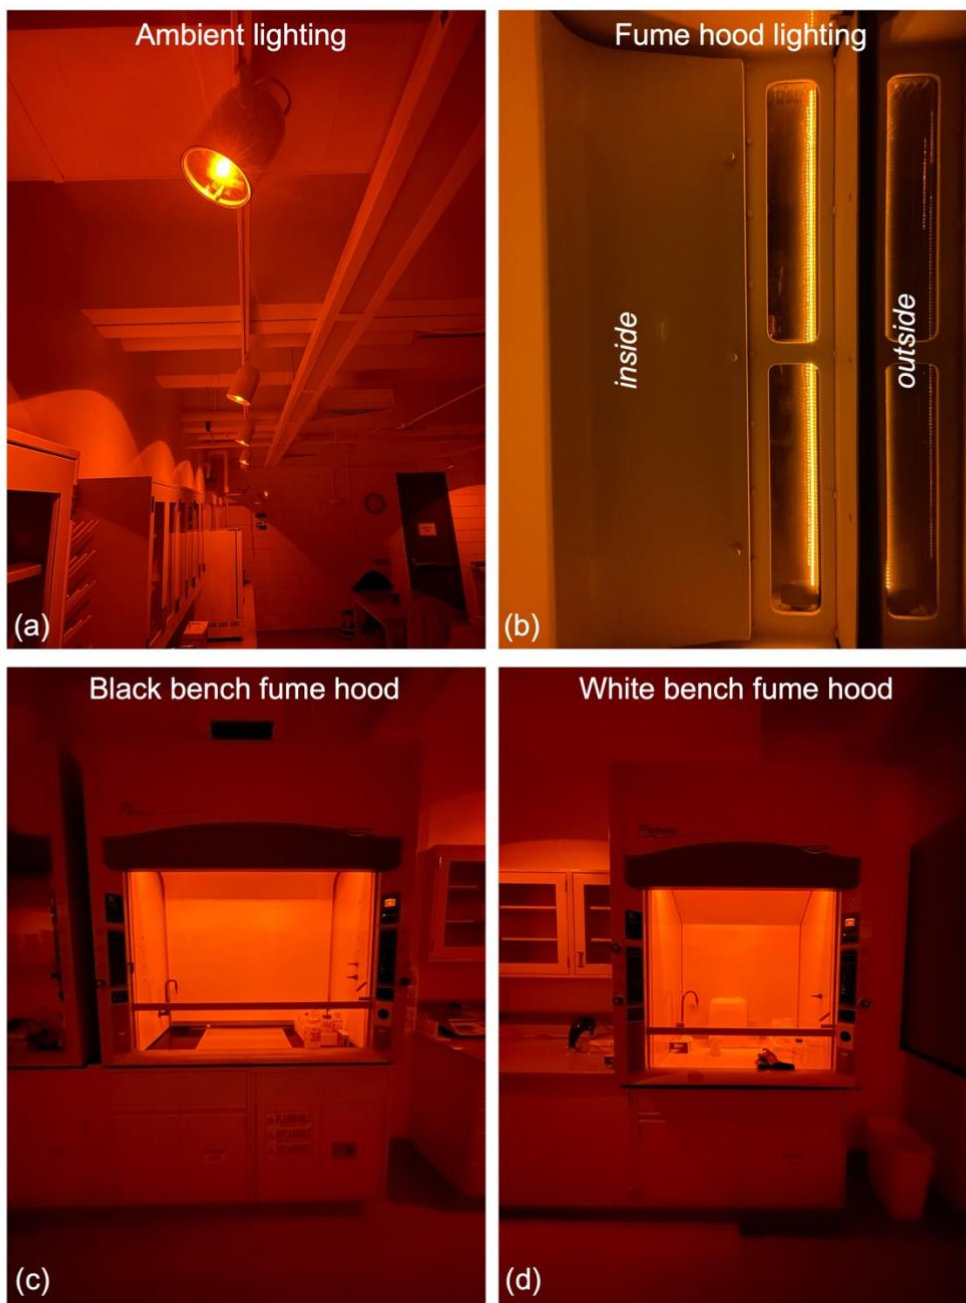
146

147 **Figure 2: Pictures of the laboratory setting in the laboratory darkroom showing the ceiling light fixture (a), and the fume hood**

148 **lighting (b-d).**

149 **4.2 Bleaching test**

150   Here we report on the capacity of our light sources in bleaching quartz and feldspar samples. Each ambient fixture

151   delivers 0.4 lux at the sample location on a benchtop. The intensity of the LED stripline in fume hood #1 was fixed at 20 %

152   and delivered 1.1 lux at the sample location on a white benchtop (referred to as I=20 % WB in Fig. 3). The intensity of the

153   LED stripline in fume hood #2 was fixed at 20 % and delivered 1.1 lux at the sample location on a black benchtop (referred

154   to as I=20 % BB in Fig. 3). The intensity of the LED stripline in fume hood #3 was fixed at 30 % and delivered 1.7 lux at the

155   sample location on a black benchtop (referred to as I=30 % BB in Fig. 3). These settings remained constant throughout the

156   experiment.

157   For all samples, we decided to report the results as dose loss because such value is directly comparable to the equivalent dose.

158   However, it is worth noting that the signal intensity loss was equal to or lower (within 2%) than the dose loss. Such a small

159   difference could be due to the fact that some aliquots were re-used multiple times over this experiment, which may have

160   affected the grain's sensitivity.

161
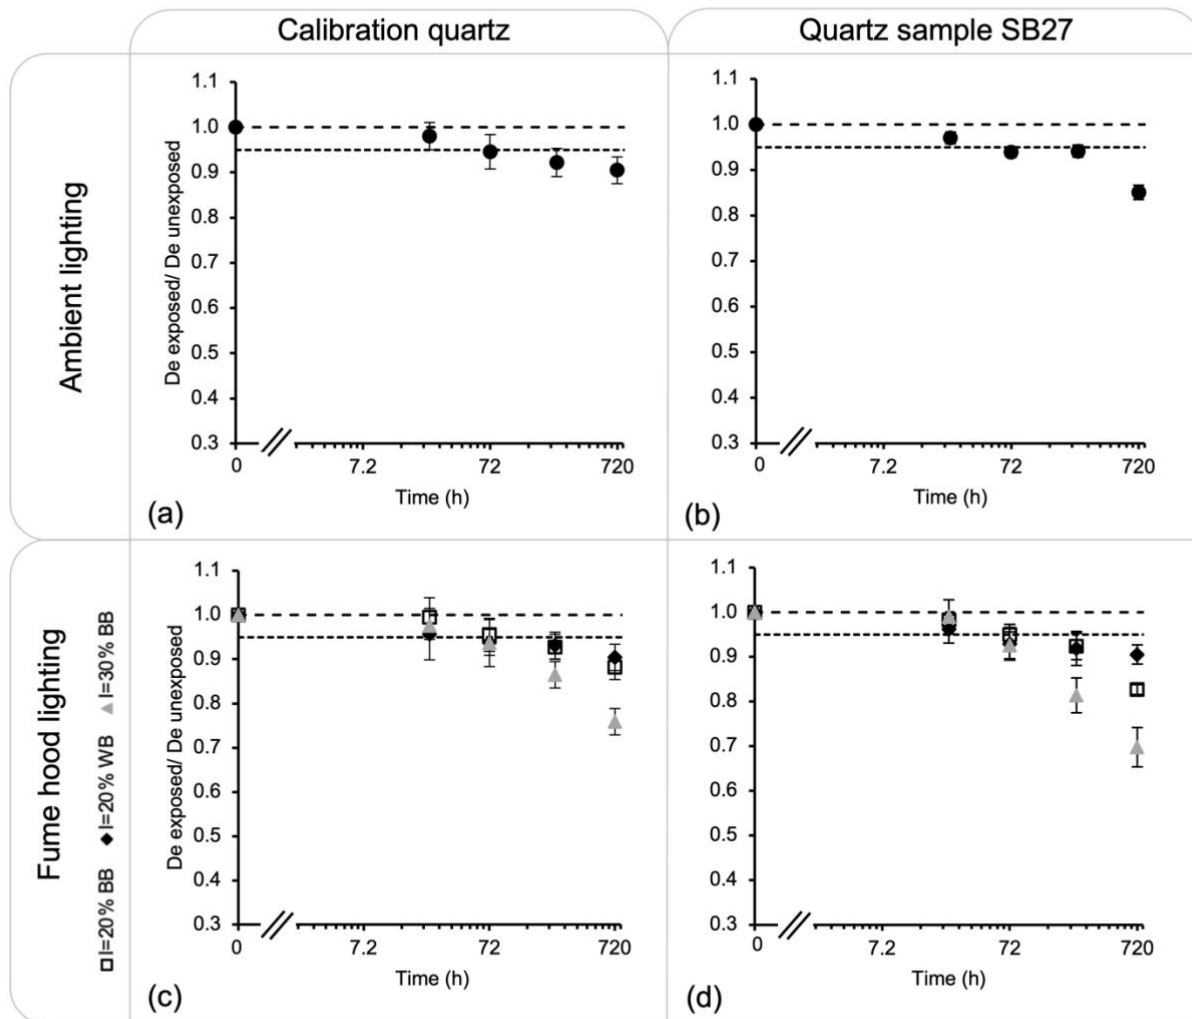
Figure 3: Ratio between the measured OSL dose from aliquots exposed to light and the measured dose from aliquots unexposed. The figures show the results from (a) the Risø calibration quartz exposed to the ceiling light fixture, (b) the quartz sample SB27 exposed to the ceiling light fixture, (c) the Risø calibration quartz exposed to fume hood lighting, and (d) the quartz sample SB27 exposed to fume hood lighting. Three aliquots were measured per exposure time. The long dashed line indicates a ratio of 1, and the dashed line indicates a loss of 5 %.

168   Figure 3a-b shows the dose decrease after exposure to the ceiling light fixture for the Risø calibration quartz and

169   sample SB27. Both samples displayed a ~3% (average) dose loss after 24 h and ~5 % after 72 h. After a substantially longer

170   exposure of 720 h, the Risø calibration quartz displayed a dose loss of ~10% and sample SB27 of ~18 %. Figure 3c-d shows

171   the remaining dose after exposure to the LED striplines within the fume hoods. For the Risø calibration quartz, the dose loss

172   is indistinguishable for the three settings after 24 h exposure. Beyond this time, however, the fume hood with the LED set to

173   an intensity of 30 % induced the fastest dose loss. The bleaching rates between the fume hood with the light intensity fixed at

174   20 % and the white benchtop or the black benchtop are indistinguishable. For both settings, the dose lost is ~1 % after 24 h

175   exposure and ~10 % after 720 h exposure. For quartz sample SB27, a similar tendency has been observed; a dose loss of ~1

176   % (average) has been recorded for the three settings after 24 h exposure. For the fume hoods with the light intensity fixed at

177   20 %, a ~10 % loss in dose was recorded after 240 h exposure, and up to 18 % after 720 h. The light fixed at 30 % intensity

178   provoked the fastest dose loss.

179   This set of measurements has been repeated on two K-rich feldspar samples. The results show more dispersion in the measured

180   dose, possibly due to the anomalous fading (all aliquots were stored and/or exposed for 30 days before measurement). Figure

181   4a-b illustrates the remaining dose after exposure to the ceiling light fixture. Before 72 h of exposure, the dose loss less than

182   ~5 % for both samples, while after 72 h, there is a drastic decrease in dose for both samples. After 720 h exposure, the dose

183   loss is between 30 to 40%.

184
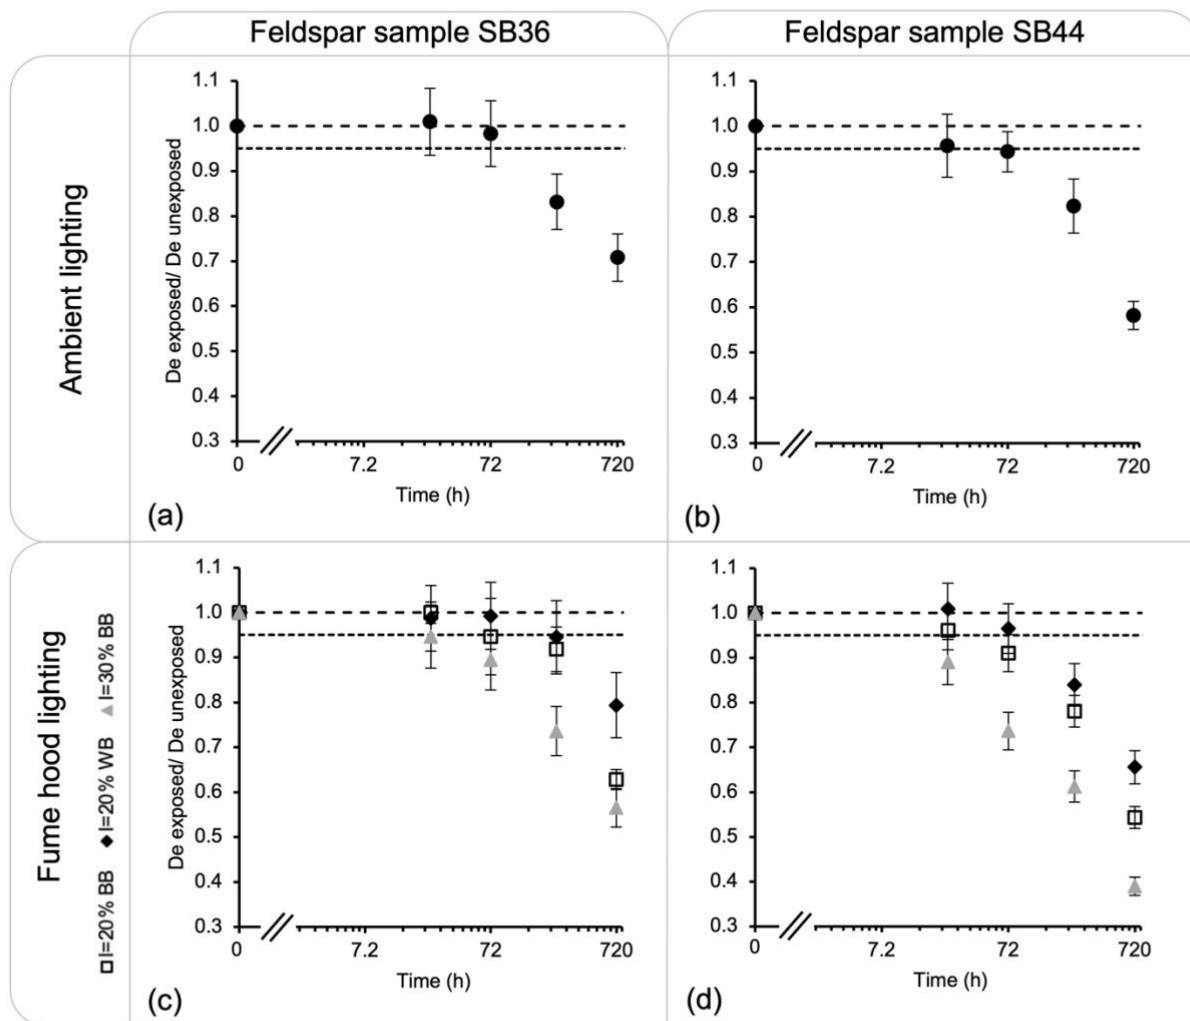
Figure 4: Ratio between the measured IR_{50} dose from aliquots exposed to light and the measured dose from aliquots unexposed.

The figures show the results from (a) the feldspar sample SB36 exposed to the ceiling light fixture, (b) the feldspar sample SB44

exposed to the ceiling light fixture, (c) the feldspar sample SB36 exposed to fume hood lighting, and (d) the feldspar sample SB44

exposed to fume hood lighting. Three aliquots were measured per exposure time. The long dashed line indicates a ratio of 1, and

the dashed line indicates a loss of 5 %.

Figure 4c-d shows the remaining dose of the initial given dose after exposure to the LED striplines within the fume hoods. The LED's set to an intensity of 30 % displayed the most rapid dose loss. After 24 h of exposure, both samples lost between 5 to 10% dose, and up to ~40 to 60 % after 720 h exposure. For the settings set at 20 % intensity, there was no loss dose recorded for sample SB36, after 24 h of exposure. The dose loss remains less than 5 % after 72 h of exposure and less than 10% after 240 h. After 720 h of exposure, the dose loss ranges between 20 to 40 %. For sample SB 44 (Fig 4d), the aliquots exposed to the LED stripline with an intensity of 30 % had a ~10 % dose loss after 24 h, and ~60 % dose loss after 720 h of exposure. For the aliquots placed under the fume hoods with an LED intensity of 20%, the dose loss was up to 5% after 24 h, 10 % after 72 h, and between 30 to 40 % after 720 h. Overall, sample SB44 bleaches faster than sample SB36. A difference in bleaching response from different K-rich feldspar samples has been observed by Sohbati et al., (2017) and interpreted as due to variation in the grain's optical transmission.

This experiment has been repeated to measure the bleaching effect of each setting on the pIR-IR$_{290}$ dose of the same K-feldspar samples (SB36 and SB44) for up to 72 h of exposure. The measured doses are undistinguishable from the given dose at 1 sigma, and therefore indicate no measurable bleaching effects of our light sources on the pIR-IR$_{290}$ dose.

Our results show the same tendency as the results reported by others (e.g., Bailif and Poolton, 1991; Spooner, 1993, 1994a, b, 2000; Sohbati et al., 2017). K-rich feldspar IRSL signal decay faster than the quartz OSL signal when exposed to yellow-orange light. The reason for such difference is, however, not fully understood. Additional analyses on well-characterized samples from different origins would be required to understand the relationship between bleaching rate and geochemical composition.

5 Conclusion

Two lighting settings have been implemented in the new Luminescence Dating Research Laboratory at Stony Brook University. For ambient lighting, ceiling fixtures were equipped with single orange LEDs. For task-oriented lighting, a dimmable orange LED stripline was mounted below the wall-mounted cabinets and inside the fume hoods. Both settings are covered with three layers of 158 Deep Orange LEE filters, and their peak wavelength is at 595 nm and 596 nm, respectively. Our bleaching tests quantified the dose loss in quartz and K-rich feldspar samples with exposure. The ambient lighting delivering 0.4 lux at the sample position induced a loss of less than 3 % in the quartz OSL dose after 24 h of exposure and between 0 to 5 % in the K-rich feldspar IR$_{50}$ doses, with no effect on their pIR-IR$_{290}$ dose. The fume hood lighting at an intensity of 20 %, delivering 1.1 lux at the sample position, induced a loss of less than 5 % in quartz OSL and K-rich feldspar IR$_{50}$ dose after 24 h of exposure. At an intensity of 30 %, the stripline of LEDs induced more rapid bleaching. Therefore, we recommend using the dimmable orange LED stripline at more than 20% intensity only in case of emergency or during lab cleaning.

Our setting is well adapted to luminescence dating darkrooms by providing a comfortable laboratory illumination for the operator, which has a minimal bleaching effect on the samples. During laboratory preparation, the samples are exposed to

ambient lighting only for a few hours, mainly during sieving and density separation, and to the fume hood lighting for a few minutes when pouring chemicals. The total light exposure to darkroom lighting should be less than 24h. In addition, extreme precautions should be taken at each step to avoid unnecessary light exposure by using non-transparent beakers when possible, covering the sample container with an opaque lid or aluminium foil, switching off the light in the fume hood when sample manipulation is not necessary, and storing the sample in an opaque container while preparing the aliquots. Finally, we plan on monitoring regularly the bleaching effect of our light sources as we work on samples from various origins.

Code/Data availability: All data are available upon request.

Author contribution: MF designed the experiments, and TG carried them out. WH and OE built the light ceiling fixture. MF designed and built the LED striplines.

Competing interests: We declare no competing interests

Acknowledgments: MF would like to thank Desmond DeLanty (architect) for designing the ceiling fixtures and installing the light sources in the laboratory.

References

Aitken, M.J. (1998) An introduction to optical dating. Oxford University Press, Oxford.

Bailiff, I. K., & Poolton, N. R. J. (1991) Studies of charge transfer mechanisms in feldspars. International Journal of Radiation Applications and Instrumentation. Part D. Nuclear Tracks and Radiation Measurements, 18(1-2), 111-118.

Hansen, V., Murray, A.S., Buylaert, J.-P., Yeo, E.Y., Thomsen, K.J. (2015) A new irradiated quartz for beta source calibration. Radiat. Meas. 81, 123-127.

Huntley, D.J., Baril, M. (2002) Yet another note on laboratory lighting. Ancient TL 20, No.2, 39-40.

Huntley, D.J., Lamothe, M. (2001) Ubiquity of anomalous fading in K-feldspars and the measurement and correction for it in optical dating. Canadian Journal of Earth Sciences 38, 1093-1106.

Lamothe, M. (1995) Using 600-650 nm light for IRSL sample preparation. Ancient TL, 13, No.1, 1-4.

Lindvall, A., Stjern, R., Alexanderson, H. (2017) Bleaching of quartz OSL signals under natural and laboratory light conditions. Ancient TL. 35.

Sohbati, R., Murray, A., Lindvold, L., Buylaert, J.-P., Jain, M. (2017) Optimization of laboratory illumination in optical dating. Quaternary Geochonology. 39. 10.1016/j.quageo.2017.02.010.

251 Sohbati, R., Kook, M., Pirtzel, L., Thomsen, K. (2021) Safelight for OSL dating laboratories: a follow-up study. Ancient
252 TL39.

253 Spooner, N.A. (1993) The validity of optical dating based on feldspar. Unpublished DPhil thesis, University of Oxford, UK

254 Spooner, N.A. (1994a). On the optical dating signal from quartz. Radiation Measurements, 23, Nos.2/3, 593-600.

255 Spooner, N.A. (1994b). The anomalous fading of infrared-stimulated luminescence from feldspars. Radiation Measurements,
256 23, Nos.2/3, 625-632.

257 Spooner, N.A., Questiaux, D., Aitken, M. (2000) The use of sodium lamps for low-intensity laboratory safelighting for optical
258 dating. 18.

259 Sutton, S.R., Zimmerman, D.W. (1978) A blue-UV absorbing filter for laboratory illumination. Ancient TL, 5, 5.

260 Thiel, C., Buylaert, J.P., Murray, A., Terhorst, B., Hofer, I., Tsukamoto, S., Frechen, M. (2011) Luminescence dating of the
261 Stratzing loess profile (Austria) - testing the potential of an elevated temperature post-IR IRSL protocol. Quat. Int. 234, 23-
262 31.

263
264

265 **Short summary.** Here, we present the lighting setting implemented in the new Luminescence Dating Research Laboratory at
266 Stony Brook University, USA. First, we performed spectral measurements on different light sources and filters. Then, we
267 measured the loss of dose in quartz and feldspar samples when exposed to various light sources and durations. Finally, we
268 conclude that our lighting setting is suitable for a luminescence darkroom laboratory, it is simple, inexpensive to build, and
269 durable.